

Fig. 1

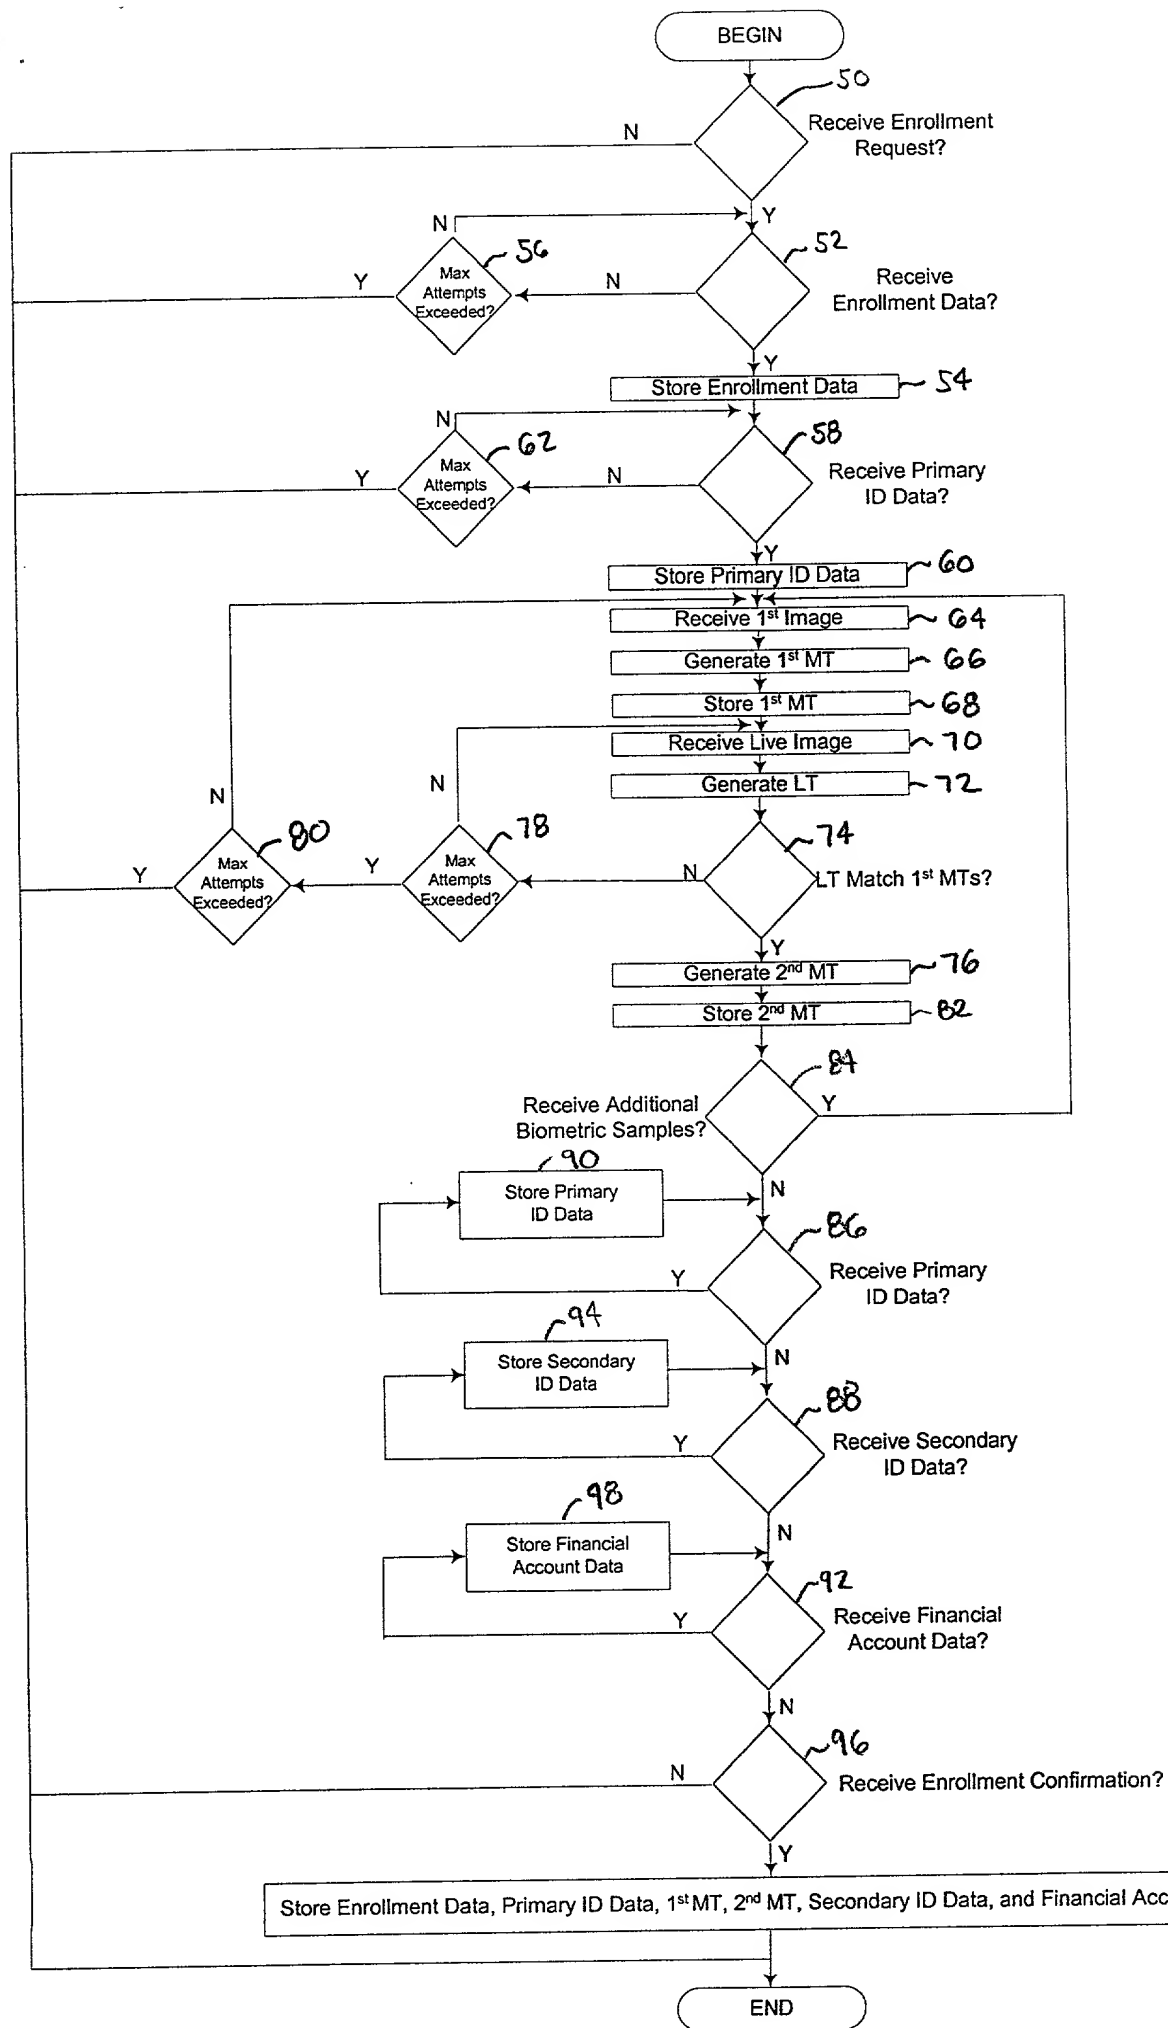


Fig. 2

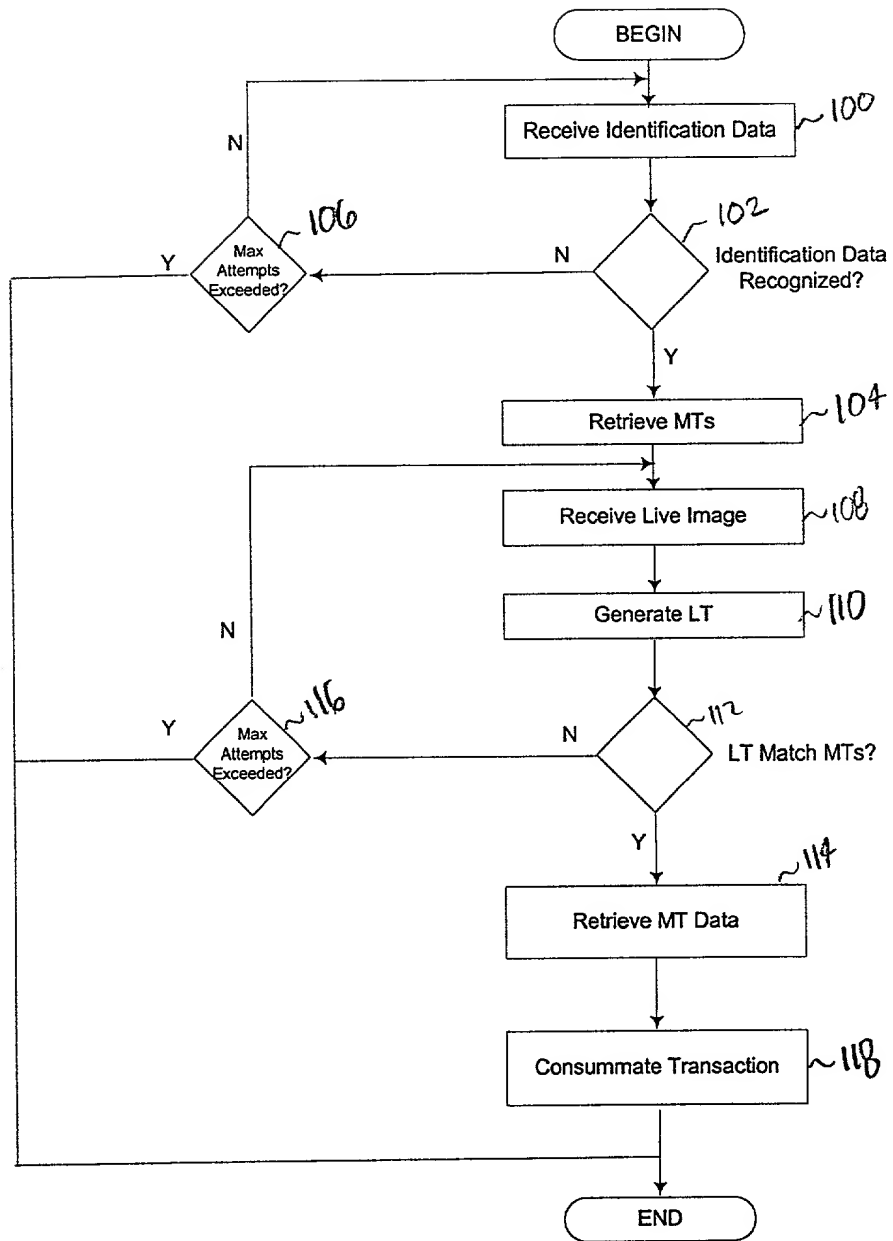


Fig. 3


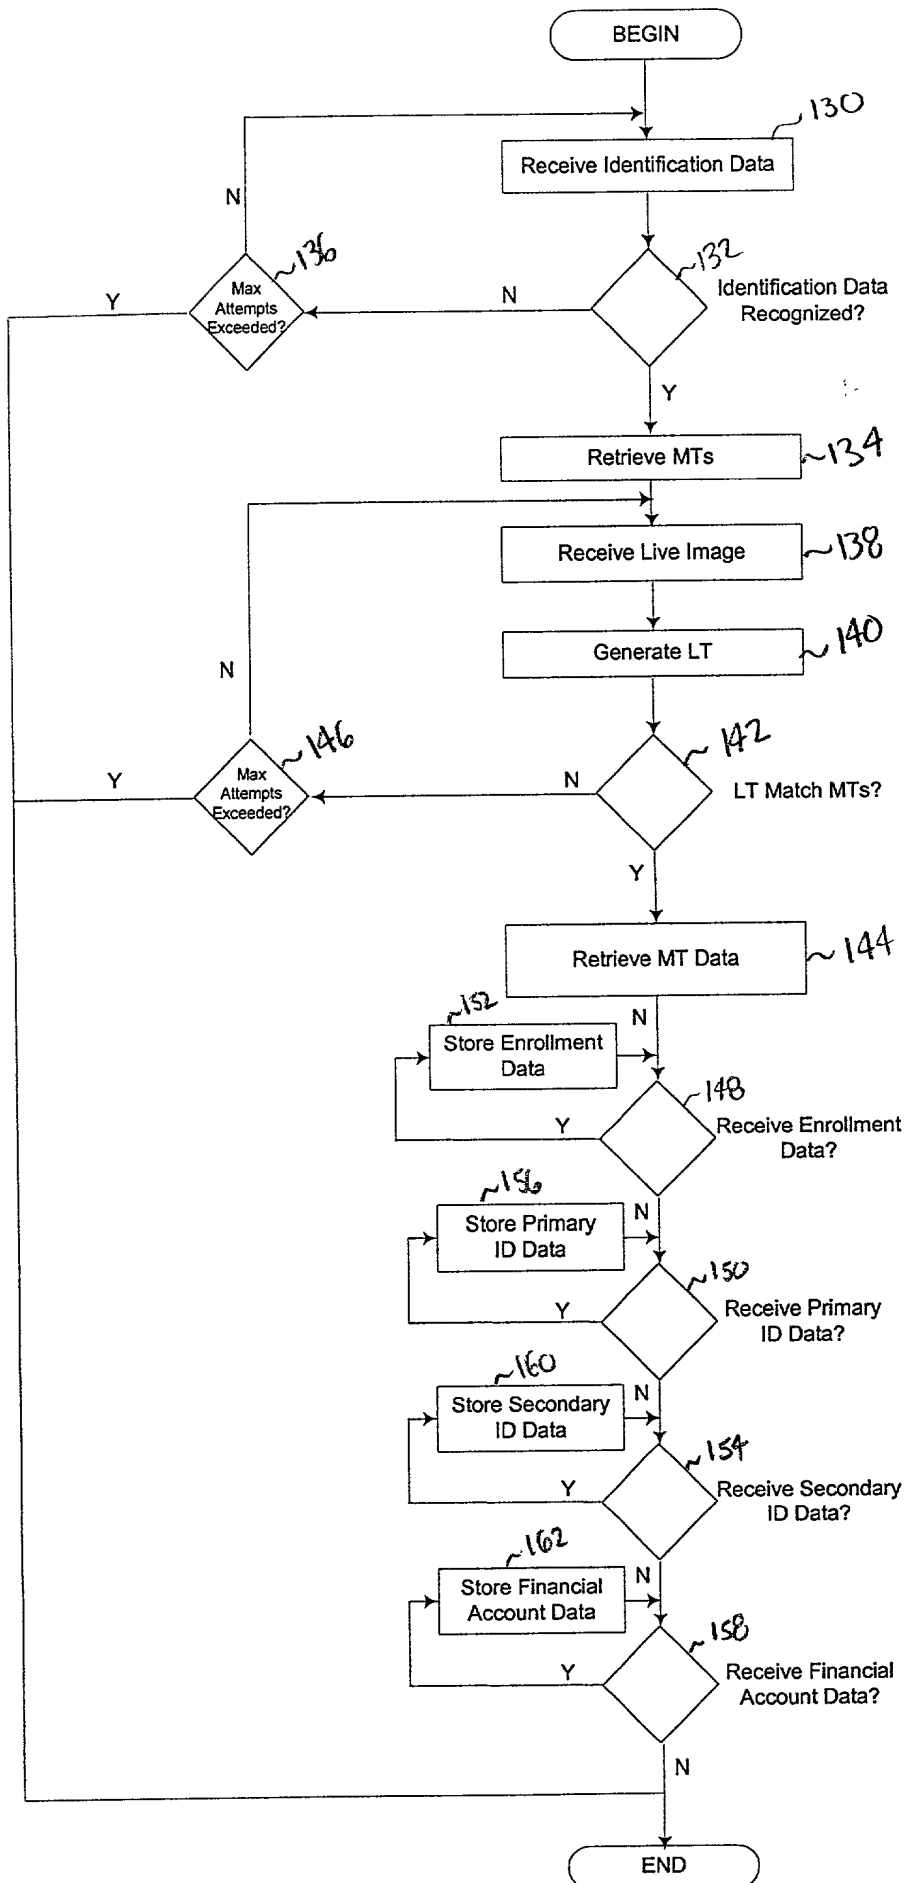


Fig. 4

Fig. 5

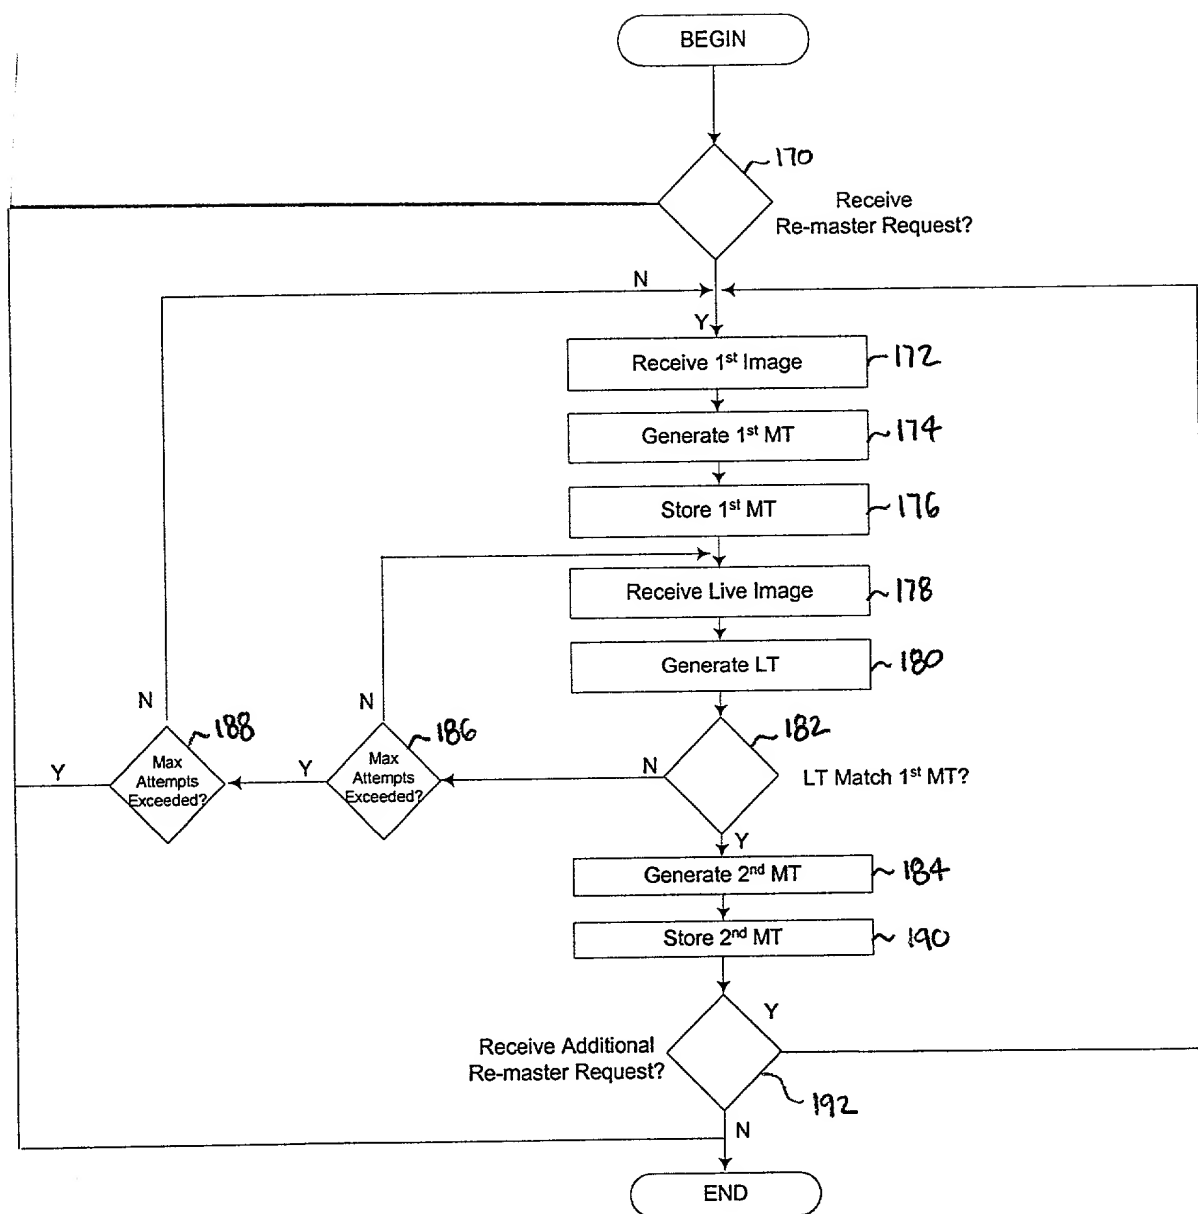

Parameter	Value	Unit
Temperature	25.0	°C
Pressure	1.0	atm
Flow rate	1.0	L/min
Concentration	0.1	mol/L
pH	7.0	
Wavelength	254	nm
Scan rate	1.0	nm/min
Integration time	1.0	s
Resolution	0.1	nm
Detector	Photodiode array	
Injection volume	10	μL
Column	C18	
Mobile phase	Water/Acetonitrile	
Gradient	0-100% ACN in 10 min	
Flow rate	1.0	mL/min
Temperature	30.0	°C
Wavelength	254	nm
Scan rate	1.0	nm/min
Integration time	1.0	s
Resolution	0.1	nm
Detector	Photodiode array	
Injection volume	10	μL
Column	C18	
Mobile phase	Water/Acetonitrile	
Gradient	0-100% ACN in 10 min	
Flow rate	1.0	mL/min
Temperature	30.0	°C
Wavelength	254	nm
Scan rate	1.0	nm/min
Integration time	1.0	s
Resolution	0.1	nm
Detector	Photodiode array	
Injection volume	10	μL
Column	C18	
Mobile phase	Water/Acetonitrile	
Gradient	0-100% ACN in 10 min	
Flow rate	1.0	mL/min
Temperature	30.0	°C
Wavelength	254	nm
Scan rate	1.0	nm/min
Integration time	1.0	s
Resolution	0.1	nm
Detector	Photodiode array	
Injection volume	10	μL
Column	C18	
Mobile phase	Water/Acetonitrile	
Gradient	0-100% ACN in 10 min	
Flow rate	1.0	mL/min
Temperature	30.0	°C
Wavelength	254	nm
Scan rate	1.0	nm/min
Integration time	1.0	s
Resolution	0.1	nm
Detector	Photodiode array	
Injection volume	10	μL
Column	C18	
Mobile phase	Water/Acetonitrile	
Gradient	0-100% ACN in 10 min	
Flow rate	1.0	mL/min
Temperature	30.0	°C
Wavelength	254	nm
Scan rate	1.0	nm/min
Integration time	1.0	s
Resolution	0.1	nm
Detector	Photodiode array	
Injection volume	10	μL
Column	C18	
Mobile phase	Water/Acetonitrile	
Gradient	0-100% ACN in 10 min	
Flow rate	1.0	mL/min
Temperature	30.0	°C
Wavelength	254	nm
Scan rate	1.0	nm/min
Integration time	1.0	s
Resolution	0.1	nm
Detector	Photodiode array	
Injection volume	10	μL
Column	C18	
Mobile phase	Water/Acetonitrile	
Gradient	0-100% ACN in 10 min	
Flow rate	1.0	mL/min
Temperature	30.0	°C
Wavelength	254	nm
Scan rate	1.0	nm/min
Integration time	1.0	s
Resolution	0.1	nm
Detector	Photodiode array	
Injection volume	10	μL
Column	C18	
Mobile phase	Water/Acetonitrile	
Gradient	0-100% ACN in 10 min	
Flow rate	1.0	mL/min
Temperature	30.0	°C
Wavelength	254	nm
Scan rate	1.0	nm/min
Integration time	1.0	s
Resolution	0.1	nm
Detector	Photodiode array	
Injection volume	10	μL
Column	C18	
Mobile phase	Water/Acetonitrile	
Gradient	0-100% ACN in 10 min	
Flow rate	1.0	mL/min
Temperature	30.0	°C
Wavelength	254	nm
Scan rate	1.0	nm/min
Integration time	1.0	s
Resolution	0.1	nm
Detector	Photodiode array	
Injection volume	10	μL
Column	C18	
Mobile phase	Water/Acetonitrile	
Gradient	0-100% ACN in 10 min	
Flow rate	1.0	mL/min
Temperature	30.0	°C
Wavelength	254	nm
Scan rate	1.0	nm/min
Integration time	1.0	s
Resolution	0.1	nm
Detector	Photodiode array	
Injection volume	10	μL
Column	C18	
Mobile phase	Water/Acetonitrile	
Gradient	0-100% ACN in 10 min	
Flow rate	1.0	mL/min
Temperature	30.0	°C
Wavelength	254	nm
Scan rate	1.0	nm/min
Integration time	1.0	s
Resolution	0.1	

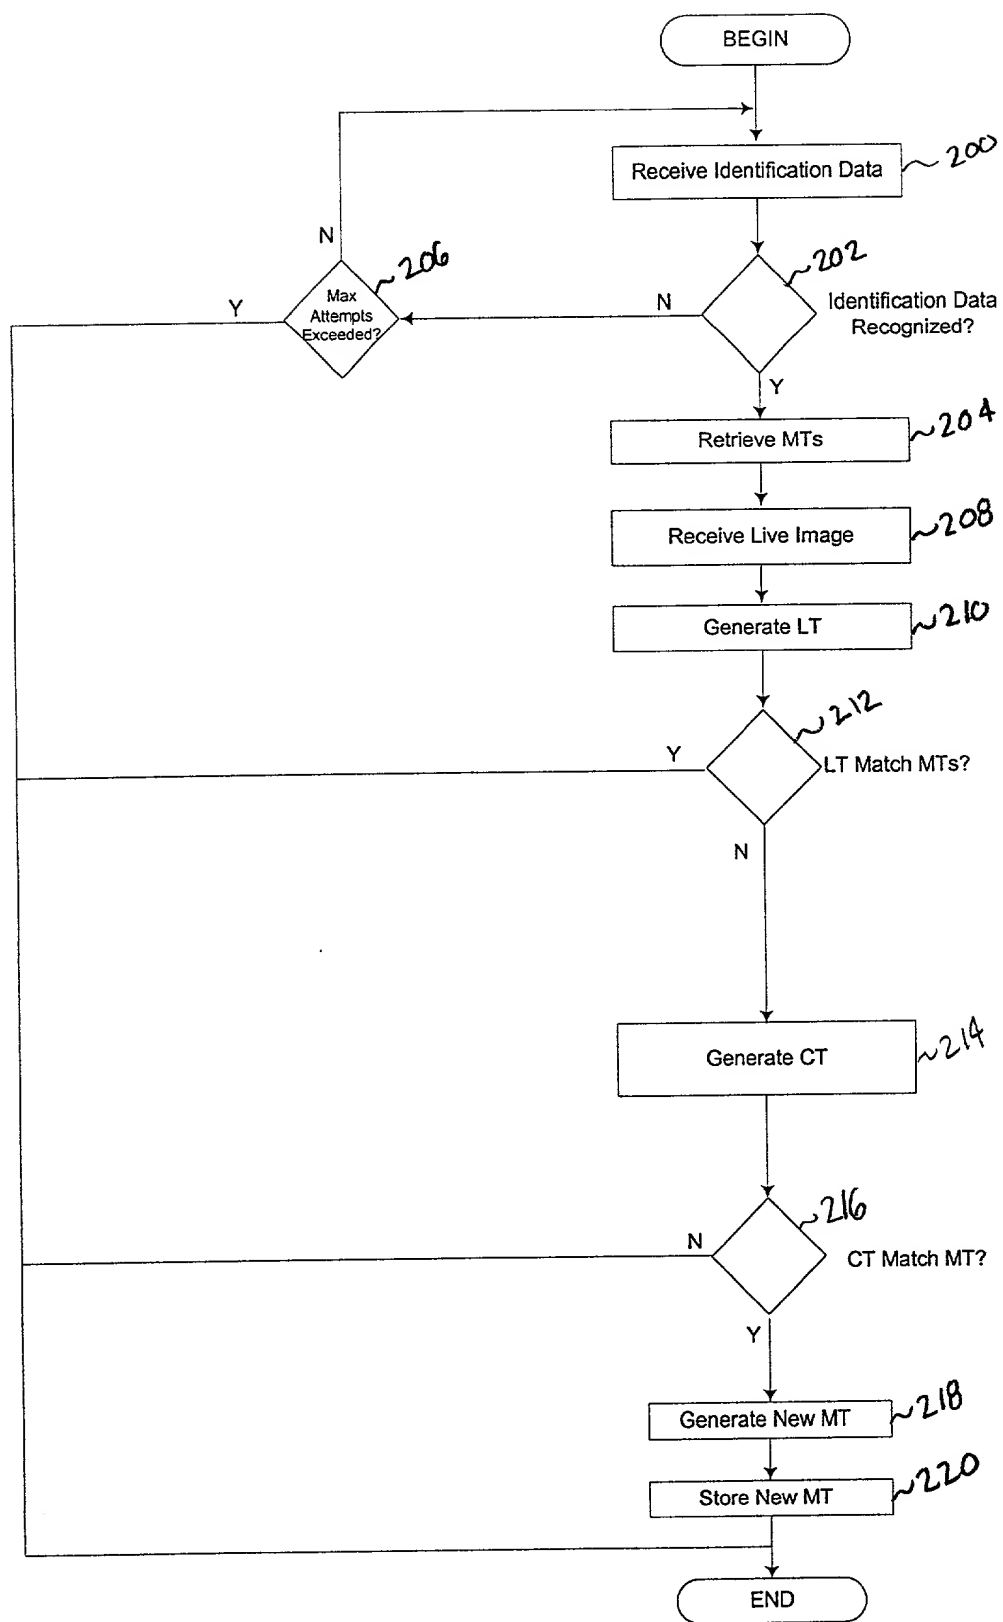


FIG. 6